


SEP 15 2010

VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

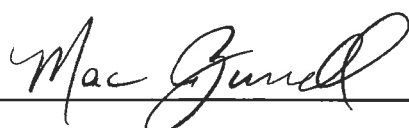		DataMaster cdm S/N		130569 ✓	
Supervisor/Operator Performing the Verification Procedure:					
A	Name	Mac Burrell		ID #	4756 ✓
				Date	9/13/2010 ✓
	Agency	Cordova Police Department		Phone #	424-6100
	Instrument Location	Cordova Police Department			
B	Alco S/N	65859 ✓	Target Value	0.081 ✓	High Pressure
					1300
	Alco Test Value Average	0.082 ✓		0.083 ✓	
		1st Alco		2nd Alco	
	Signature				
(OVER)					


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

(Do Not write in the area below)



- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 9th day of Nov, 2010.


 Daniel L. Nicholas
 Notary Public, State of Alaska
 Commission Expires with Office

(Notary Seal Stamp)

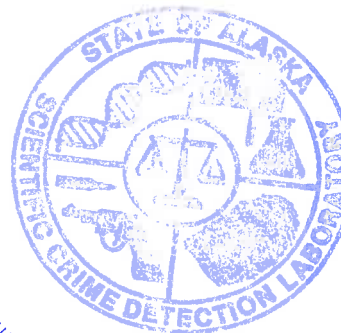

VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

DataMaster cdm S/N

130569

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

SEPTEMBER 13, 2010

OPERATOR'S NAME:

BURRELL/M

OPERATOR'S NUMBER: 4756

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME: MI

M

O.L. #: 1

DEPT/AGENCY: CDV1

ORCE/REPORT: 091210

TEST TYPE: V

ALCO TARGET VALUE: .001

ALCO S/N: 65859

--- BREATH ANALYSIS ---

.001 ADJUSTED FOR 30.37 in

ALCO TARGET .002 15:49

BLANK TEST .000 15:50

INTERNAL STANDARD VERIFIED 15:50

ALCO TV 30.37 in .002 15:50

BLANK TEST .000 15:51

SUBJECT SAMPLE .000 15:52

BLANK TEST .000 15:53

ALCO TV 30.37 in .003 15:53

BLANK TEST .000 15:54

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

SEPTEMBER 13, 2010

TIME 15:46

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 49c

BAROMETER: 30.37 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!""##&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcde'ghijklmno
pqrstuvwxyz{|}~"